Ultrasonic Flowmeters sitrans f us sono 3100

Operating instructions • 06/2010



SITRANS F



SIEMENS

| Introduction | 1 |
|------------------------|---|
| Safety notes | 2 |
| Description | 3 |
| Installing/Mounting | 4 |
| Electrical connection | 5 |
| Maintenance and repair | 6 |
| | 7 |
| Technical data | • |
| Appendix A | A |

SITRANS F

Ultrasonic flowmeters SITRANS F US SONO 3100

Operating Instructions

Sensor type SONO 3100 DN 100 \dots DN 1200 for use with transmitter type FUS060

Legal information

Warning notice system

This manual contains notices you have to observe in order to ensure your personal safety, as well as to prevent damage to property. The notices referring to your personal safety are highlighted in the manual by a safety alert symbol, notices referring only to property damage have no safety alert symbol. These notices shown below are graded according to the degree of danger.

indicates that death or severe personal injury will result if proper precautions are not taken.

WARNING

indicates that death or severe personal injury may result if proper precautions are not taken.

with a safety alert symbol, indicates that minor personal injury can result if proper precautions are not taken.

CAUTION

without a safety alert symbol, indicates that property damage can result if proper precautions are not taken.

NOTICE

indicates that an unintended result or situation can occur if the corresponding information is not taken into account.

If more than one degree of danger is present, the warning notice representing the highest degree of danger will be used. A notice warning of injury to persons with a safety alert symbol may also include a warning relating to property damage.

Qualified Personnel

The product/system described in this documentation may be operated only by **personnel qualified** for the specific task in accordance with the relevant documentation for the specific task, in particular its warning notices and safety instructions. Qualified personnel are those who, based on their training and experience, are capable of identifying risks and avoiding potential hazards when working with these products/systems.

Proper use of Siemens products

Note the following:

WARNING

Siemens products may only be used for the applications described in the catalog and in the relevant technical documentation. If products and components from other manufacturers are used, these must be recommended or approved by Siemens. Proper transport, storage, installation, assembly, commissioning, operation and maintenance are required to ensure that the products operate safely and without any problems. The permissible ambient conditions must be adhered to. The information in the relevant documentation must be observed.

Trademarks

All names identified by ® are registered trademarks of the Siemens AG. The remaining trademarks in this publication may be trademarks whose use by third parties for their own purposes could violate the rights of the owner.

Disclaimer of Liability

We have reviewed the contents of this publication to ensure consistency with the hardware and software described. Since variance cannot be precluded entirely, we cannot guarantee full consistency. However, the information in this publication is reviewed regularly and any necessary corrections are included in subsequent editions.

Table of contents

| 1 | Introdu | uction | 5 |
|---|----------|---|----|
| | 1.1 | Items supplied | 5 |
| | 1.2 | History | 5 |
| | 1.3 | Further Information | 6 |
| 2 | Safety | / notes | 7 |
| | 2.1 | Laws and directives | 7 |
| | 2.2 | Installation in hazardous area | 8 |
| | 2.3 | Certificates | 9 |
| 3 | Descri | iption | 11 |
| | 3.1 | System components | 11 |
| | 3.2 | Design | 11 |
| | 3.3 | Theory of operation | 13 |
| 4 | Installi | ing/Mounting | |
| | 4.1 | Installation safety precautions | 15 |
| | 4.2 | Determining a location | 16 |
| | 4.3 | Orienting the sensor | 19 |
| | 4.4 | Mounting the sensor | |
| 5 | Electri | ical connection | 21 |
| | 5.1 | Step 1: Transducer wiring | 21 |
| | 5.2 | Step 2: Wiring transducer and transmitter | 23 |
| 6 | Mainte | enance and repair | |
| | 6.1 | Maintenance | 25 |
| | 6.2 | Recalibration | |
| | 6.3 | Unit repair | |
| | 6.4 | Technical support | |
| | 6.5 | Application information guide | |
| | 6.6 | Return procedures | |
| 7 | Techn | nical data | |
| | 7.1 | Coaxial cable specifications | |
| | 7.2 | Pressure and temperature rating | 31 |
| | 7.3 | Reference conditions | |
| | 7.4 | Dimensions and Weight | |

| Α | Append | ix A | . 37 |
|---|--------|----------------------------------|------|
| | A.1 | Sizing table (DN 100 to DN 1200) | . 37 |
| | A.2 | Ordering | . 38 |
| | Index | | . 39 |

Introduction

These instructions contain all the information you need for using the device.


The instructions are aimed at persons mechanically installing the device, connecting it electronically, configuring the parameters and commissioning it as well as service and maintenance engineers.

Note

It is the responsibility of the customer that the instructions and directions provided in the manual are read, understood and followed by the relevant personnel before installing the device.

1.1 Items supplied

- SITRANS F US SONO 3100
- SITRANS F literature CD
- Quick Start guide
- Calibration report
- Transducer coaxial cable (4 pcs)
- Transmitter type FUS060 (not shown)



Note

Scope of delivery may vary, depending on version and add-ons.

Note

Handle with care!

Impact and shock can damage the piezeoelectric crystal located in the transducers.

1.2 History

The contents of these instructions are regularly reviewed and corrections are included in subsequent editions. We welcome all suggestions for improvement.

1.3 Further Information

The following table shows the most important changes in the documentation compared to each previous edition.

| Edition | Remarks |
|---------|---|
| 12/2007 | SITRANS F US Ultrasonic flowmeter Sensor type SONO 3100 DN 100 DN 1200 for use with transmitter type FUS060 (Operating manual, revision 3.) |
| 06/2010 | Revision 4. Contents restructured. |

Note

A flowmeter system consists of a sensor (SONO 3100) and a transmitter (FUS060).

These Operating Instructions only cover the sensor part of the system. The transmitter FUS060 has a separate manual, which is available on the SITRANS F literature CD-ROM and on the flow documentation homepage (http://www.siemens.com/flowdocumentation)

1.3 Further Information

The contents of these Operating Instructions shall not become part of or modify any prior or existing agreement, commitment or legal relationship. All obligations on the part of Siemens AG are contained in the respective sales contract which also contains the complete and solely applicable warranty conditions. Any statements contained herein do not create new warranties or modify the existing warranty.

Product information on the Internet

The Operating Instructions are available on the CD-ROM shipped with the device, and on the Internet on the Siemens homepage, where further information on the range of SITRANS F flowmeters may also be found:

Product information on the internet (http://www.siemens.com/flow)

Worldwide contact person

If you need more information or have particular problems not covered sufficiently by the operating instructions, please get in touch with your contact person. You can find contact information for your local contact person on the Internet:

Local contact person (http://www.automation.siemens.com/partner)

Safety notes

Correct, reliable operation of the product requires proper transport, storage, positioning and assembly as well as careful operation and maintenance. Only qualified personnel should install or operate this instrument.

Note

Alterations to the product, including opening or improper repairs of the product, are not permitted.

If this requirement is not observed, the CE mark and the manufacturer's warranty will expire.

2.1 Laws and directives

General requirements

Installation of the equipment must comply with national regulations. For example EN 60079-14 for installation in hazardous location in the European Community.

Instrument safety standards

The device has been tested at the factory, based on the safety requirements. In order to maintain this condition over the expected life of the device the requirements described in these Operating Instructions must be observed.

CAUTION

Material compatibility

The meters have been designed according to EN 13480 with an additional corrosion layer of approx. 1 mm for steel sensors. Stainless steel transducer parts do not have an additional layer.

It is the responsibility of the customer to ensure that the medium is compatible with the sensor construction material. The full responsibility for the selection rests with the customer and Siemens Flow Instruments can take no responsibility for any failure due to material incompatibility.

2.2 Installation in hazardous area

CE marked equipment

The CE-mark symbolizes the compliance of the device with the following directives:

- EMC directive 2004/108/EC
- Low voltage directive 2006/95/EC
- Pressure equipment directive (PED/DGRL) 97/23/EC
- ATEX Directive 94/9/EC

2.2 Installation in hazardous area

WARNING

Equipment used in hazardous areas must be Ex-approved and marked accordingly. It is required that the special conditions for safe use provided in the manual and in the Ex certificate are followed!

Hazardous area approvals

This flowmeter (SONO 3100 with FUS060) is approved for use in hazardous area and has the following approvals:

- Transmitter (FUS060): II 2G Ex dem [ia/ib] IIC T6/T4/T3 (Only approved for use with SONO 3100 Ex-i)
- Sensor (SONO 3100 Ex-i approved version): II 2G Ex ib IIC T6/T4/T3 (Only approved for use with FUS060 Ex-version)
- Sensor (SONO 3100 Ex d approved version): II 2G EEx d IIC T3-T6 (Only approved for use with FUS060 non Ex-version installed in safe zone)

Make sure the hazardous area approval is suitable for the environment in which the device will be installed.

Temperature specifications for use in hazardous area

Table 2-1 Hazardous area temperature specifications for SONO 3100 Ex-i approved versions

| Temperature class | Max. surface temperature | Media temperature | Ambient temperature |
|-------------------|--------------------------|-------------------|---------------------|
| Т3 | +200°C | -10 200°C | -20 +60°C |
| T4 | +135°C | -10 135°C | -20 +60°C |
| Т5 | +100°C | -10 100°C | -20 +60°C |
| Т6 | +85°C | -10 85°C | -20 +60°C |

| Temperature class | Max. surface temperature | Media temperature | Ambient temperature |
|-------------------|--------------------------|-------------------|---------------------|
| Т3 | +200°C | -10 200°C | -20 +180°C |
| T4 | +135°C | -10 135°C | -20 +125°C |
| T5 | +100°C | -10 100°C | -20 +90°C |
| Т6 | +85°C | -10 85°C | -20 +75°C |

Table 2-2 Hazardous area temperature specifications for SONO 3100 Ex-d approved versions

Media temperature specifications

Make sure that media temperature specifications indicated on the device type plate / label will not be exceeded.

Hazardous area safety requirements

WARNING

It is required that:

- Electrical connections are in accordance with EN60079-14 (Installing Electrical Systems in Explosion Hazardous Areas).
- Appropriate cable connectors are used for the output circuits:
 - Intrinsically safe: blue and / or metal (nickle plated brass)
 - Non-intrinsically safe: gray or black
- Protective earth terminals (PE) on both sensor and transmitter are connected (min. 4mm²).

2.3 Certificates

Certificates are posted on the Internet and on the manual collection shipped with the device.

See also

Certificates (http://www.siemens.com/processinstrumentation/certificates)

Safety notes

2.3 Certificates

Description

SITRANS F US ultrasonic flowmeters measure flow in standard volumetric units. Measurement is independent of changes in liquid temperature, density, pressure and conductivity. A time of flight flowmeter is designed for use on single phase liquids.

They are designed for measurement of:

- Volume flow rate
- Limit monitoring
- Total volume
- Sound velocity in the media

3.1 System components

| | Table 3-1 | System components, | , SONO 3100 with FUS060 |
|--|-----------|--------------------|-------------------------|
|--|-----------|--------------------|-------------------------|

| Sensor | Transmitter | Outputs | Measurement |
|------------------|-------------|------------------|----------------------|
| SONO 3100 | FUS060 | Analog with HART | Volume flow rate |
| DN 100 - DN 1200 | | Frequency-/pulse | Total volume |
| (40" - 480") | | • Relay | Mass flow rate |
| | | or | Total mass |
| | | Profibus PA | Sound velocity |
| | | Frequency-/pulse | Error indication |
| | | | Limit monitoring |
| | | | Ultrasonic Amplitude |

3.2 Design

SITRANS F US SONO 3100 with FUS060 is designed for measuring the flow velocity of liquids in full pipes. Satisfactory function of the ultrasonic flowmeter depends on a low sound attenuation of the medium and a well-defined and stable flow profile.

The sensor SONO 3100 with transmitter FUS060 remote mounted measures with a high accuracy (better than $\pm 0.5\%$ of reading over a wide measuring range).

Description

3.2 Design



Figure 3-1 SITRANS F US SONO 3100 (shown without FUS060)

The following table shows the properties of the ultrasonic flowmeter system SITRANS F US SONO 3100 with the transmitter type FUS060

Transducer SONO 3200

The transducer type SONO 3200 is available in two variants:


• Flange type:

The transducer has a DIN flange with a groove for fitting to a corresponding flange welded onto the pipe.

• O-ring type:

The transducer has a screwed union connection for fitting in a counterflange welded onto the pipe. The union and pipe are sealed with an O-ring.


Transducers are constructed in three parts:

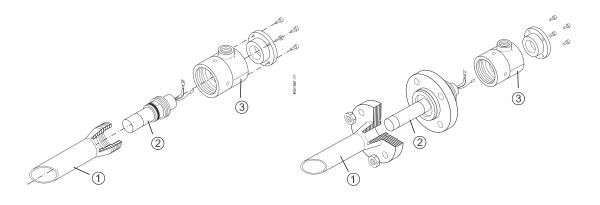

- ① Transducer holder
- (2) Terminal housing
- (3) Transducer element

SONO 3200 exploded view

Transducer element

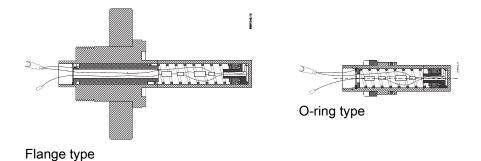

The terminal box, transducer element and insert are identical in both versions.

The insert, consisting of a spring and piezo crystal, can be removed from the transducer element during operation. No draining is necessary as the transducer element remains in the pipe. When exchanging the transducer insert everything must be kept extremely clean to avoid dirt between piezo and window.




Figure 3-2 Transducer element insert

3.3 Theory of operation

Physical principle

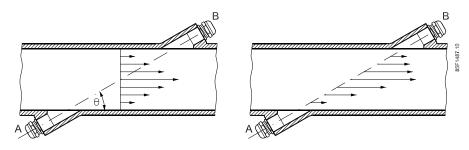


Figure 3-3 Velocity distribution along sound path

A sound wave travelling in the same direction as the liquid flow arrives at point B from point A in a shorter time than the sound wave travelling against the direction of flow (from point B to A).

The difference in sound transit time indicates the flow velocity in the pipe.

3.3 Theory of operation

Since delay time is measured at short intervals both in and against flow direction, temperature has no influence on measurement accuracy.

SITRANS F US flowmeters

In SITRANS F US flowmeters the ultrasonic transducers are placed at an angle θ in relation to the pipe axis. The transducers function as transmitters and receivers of the ultrasonic signals. Measurement is performed by determining the time the ultrasonic signal takes to travel with and against the flow. The principle can be expressed as follows:

| v | = | $K\times \left(t_{B,A} - t_{A,B} \right) / \left(t_{A,B}\times t_{B,A} \right) = K\times \Delta t / t^2$ |
|---|---|--|
| v | = | Average flow velocity |
| t | = | Transit time |
| K | = | Proportional flow factor |

This measuring principle offers the advantage that it is independent of variations in the actual sound velocity of the liquid, i.e. independent of the temperature.

The Proportional factor K is determined by wet calibration or calculated by "Auto" in case of manual programming of mechanical geometrical pipe data (SONOKIT only). The transducer angle (Θ), distance between sensors (L) and pipe dimension (Di) are shown in the figure below.




Figure 3-4 Measuring principle

The ultrasonic signal is sent directly between the transducers. The advantage gained sending signals from point to point is an extremely good signal strength.

Installing/Mounting

The installation of the sensor has 3 steps:

- 1. Selecting the measuring site (Page 16)
- 2. Orienting the sensor (Page 19)
- 3. Mounting the sensor (Page 20)

Ambient conditions



- SITRANS F flowmeters are suitable for in- and outdoor installations.
- The SONO 3100 has the following temperature specifications:
 - Media/surface temperature: -10 to 160 °C (14 to 320 °F)
 - Ambient temperature: -20 to +60 °C (-4 ... +140 °F)
 - Storage –40 °C to 85 °C (14 to 185 °F).
- The enclosure rating is IP67 (NEMA 4X/6) or better.

CAUTION

Make sure that pressure and temperature specifications indicated on the device type plate / label will not be exceeded.

Note

In case of large temperature differences between medium and environment, the sensor must be isolated to avoid 2-phase flow which will result in inaccurate measuring results

WARNING

Installation in hazardous location

Special requirements apply to the location and interconnection of sensor and transmitter. See "Installation in hazardous area" (Page 8)

4.1 Installation safety precautions

WARNING

In applications with working pressures/media that can be dangerous to people, surroundings, equipment or others in case of pipe fracture, we recommend that special precautions such as special placement, shielding or installation of a security guard or a security valve are taken when the sensor is mounted.

4.2 Determining a location

- Ensure that stresses and loading caused by e.g. earthquakes, traffic, high winds and fire damage if appropriate are taken into account during installation.
- Ensure that the flowmeter is installed such that it does not act as a focus for pipeline stresses. External loadings are not taken into account in the flowmeter design.
- Provide adequate protection to minimise any risk of contact with hot surfaces.

WARNING


Prevent personal injuries by assuring that operation below pressure guards cannot take place, if working with vacuum or fluids boiling readily.


4.2 Determining a location

CAUTION


The sensor must always be completely filled with liquid.

• Locate the flowmeter in U-shaped pipes if pipes are only partially filled or have free outlet.





- Avoid the following installations:
 - Installation at the highest point of the pipe system
 - Installation in vertical pipes with free outlet

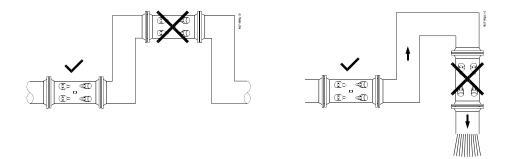

Inlet / outlet conditions

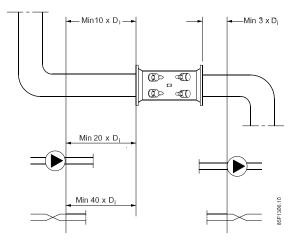


Figure 4-1 Inlet / outlet conditions

- Ensure that inlet and outlet are straight
- Ensure sufficient distance between meter and bends, pump and valves (see the table below).
- Install valves influencing the flow profile after the flowmeter. The only exception is installation of the sensor in a vertical pipe (upwards flow direction). In installations in a vertical pipe a valve below the sensor is required to allow zero-point adjustment

Note

Select a valve not altering flow when fully opened.

| | Table 4- 1 | Recommended inlet / | outlet conditions |
|--|------------|---------------------|-------------------|
|--|------------|---------------------|-------------------|

| Recommended inlet / outlet | |
|-----------------------------|--------------------------|
| 90° bend | Min. 10 x D _i |
| Fully opened valve | Min. 10 x D _i |
| Partially opened valve | Min. 40 x D _i |
| 2 x 90° bends in same plane | Min. 15 x D _i |
| 2 x 90° bends in two planes | Min. 20 x D _i |
| Outlet | 3 x Di |


Note

By more than one bend, the optimal inlet is min. 40 × pipe diameter.

4.2 Determining a location

Installation with pipe reducers

The flowmeter can be installed between two reducers.

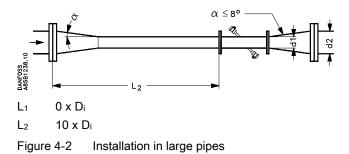

At 8° the following pressure drop curves apply. The curves are applicable to water.

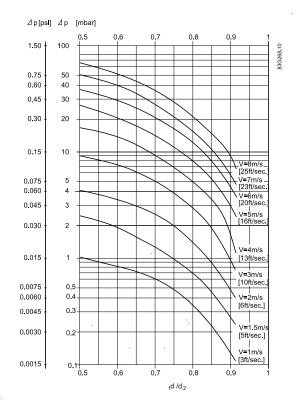


Figure 4-3 Pressure loss by use of pipe reducers

4.3 Orienting the sensor


Flow direction


The flow direction is indicated with the "+" on the double arrow on the sensor.


Orienting the sensor

SITRANS F US SONO 3100 operates in any orientation, but Siemens Flow Instruments recommends orienting the sensor as follows:

1. Vertical orientation with an upwards flow in order to minimize the effect of gas / air bubbles in the media









Vertical installation, downwards flow

1. Horizontal orientation with transducers installed horizontally



Horizontal installation, transducers oriented horizontally



Horizontal installation, transducers oriented vertically

4.4 Mounting the sensor

Measurement of liquids containing abrasive or other particles

In order to minimize wear, a vertical installation with an upwards flow is recommended.

4.4 Mounting the sensor

- Install the sensor in rigid pipelines in order to support the weight of the meter.
- Centre the connecting pipelines axially in order to assure a stress-free installation.
- Centre the flowmeter in relation to pipe flanges and gaskets.
- Install two supports or hangers symmetrically and stress-free in close proximity to the process connections.



Gas / air bubbles in the liquid

Avoid the accumulation of large quantities of air in the sensor as these will affect measurement. When air is present, installation of an air separator upstream of the meter is recommended.

Electrical connection

The following contains a short description of how to connect the sensor to the transmitter SITRANS FUS060. For more information, please refer to the relevant Operating Instructions of the transmitter.

Only qualified personnel may carry out work on the electrical connections.

WARNING


Use in hazardous locations

Before opening the terminal box check that:


- No explosion hazard exists
- A fire department permission certificate has been issued
- All connection leads are potential free

Special requirements apply to the location and interconnection of sensor and transmitter. See "Installation in hazardous area" (Page 8)

5.1 Step 1: Transducer wiring



Electrical connection of transducer



- 1. Remove the lid of the terminal housing
- 2. Connect the wire without a spade terminal to position 2
- 3. Connect the wire with a spade terminal to the transducer housing by means of position 3.
- 4. Connect the wire of the transducer coax cable to position 1.

5.1 Step 1: Transducer wiring

- 5. Fix the shield wire coax cable to the cable clip in position 4.
- 6. Remount the lid.



Avoid stress on the connection wires when passing them through the terminal box.

Disassembling the terminal box

- Loosen the wires from the connection board. It is not necessary to remove the transducer cable.
- Support the terminal box while loosening the union. Then remove the terminal box from the transducer holder.



Turning the terminal box can damage the wires to the crystals

Electrical connection

5.2 Step 2: Wiring transducer and transmitter

5.2 Step 2: Wiring transducer and transmitter

Wire transducer cables and transmitter as follows:

1. Connect the 4 transducer cables at the FUS060 transmitter as shown below (terminal plug 1B, 1A, 2B and 2A):

Push the SMB-plug cable ends carefully through the cable glands, plug them in and fix them by using the glands.

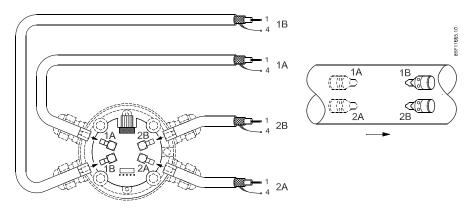


Figure 5-1 Electrical connection of SONO 3100 and FUS060

2. Ensure that transducer cables are not overbent. Minimum cable bend radius is 50 mm





Figure 5-2 Minimum cable bend radius

3. Tighten the cable glands to obtain optimum sealing. The gaskets must protrude along the cable



Cable sealing, incorrect

Cable sealing, correct

5.2 Step 2: Wiring transducer and transmitter

4. Ground transmitter and sensor for optimal performance.

Grounding

A direct ground connection of transmitter and sensor is recommended.

WARNING

Use in hazardous area

Connect protective earth terminals (PE) on both sensor and transmitter (min. 4mm²)

Maintenance and repair

6.1 Maintenance

The device is maintenance-free, however, a periodic inspection according pertinent directives and regulations must be carried out.

An inspection can include check of:

- Ambient conditions
- Seal integrity of the process connections, cable entries, and cover screws
- Reliability of power supply, lightning protection, and grounds

6.2 Recalibration

Siemens Flow Instruments offers to recalibrate the sensor. The following calibrations are offered as standard:

- Standard matched pair calibration
- Accredited matched pair calibration

Note

For recalibration the transmitter must always be returned with the sensor

6.3 Unit repair

CAUTION

Repair and service must be carried out by Siemens authorized personnel only.

Note

Siemens Flow Instruments defines sensors as non-repairable products.

6.4 Technical support

If you have any technical questions about the device described in these Operating Instructions and do not find the right answers, you can contact Technical Support:

- Via the Internet using the **Support Request:** Support request (http://www.siemens.com/automation/support-request)
- Phone: +49 (0)911 895 7222

Further information about our technical support is available in the Internet at Technical support (http://support.automation.siemens.com/WW/view/en/16604318)

Service & Support on the Internet

In addition to our documentation, we offer a comprehensive knowledge base online on the Internet at:

Service and support (http://www.siemens.com/automation/service&support)

There you will find:

- The latest product information, FAQs, downloads, tips and tricks.
- Our newsletter, providing you with the latest information about your products.
- A Knowledge Manager to find the right documents for you.
- Our bulletin board, where users and specialists share their knowledge worldwide.
- You can find your local contact partner for Industry Automation and Drives Technologies in our partner database.
- Information about field service, repairs, spare parts and lots more under "Services."

Additional Support

Please contact your local Siemens representative and offices if you have additional questions about the device

Find your contact partner at:

Local contact person (http://www.automation.siemens.com/partner)

6.5 Application information guide

In case the device needs service, the factory will typically request information about application and flowmeter.

The following tables can be used as a preparation guide before taking contact to Siemens.

Note

Sketch

It is recommended to prepare a sketch of the installation / application.

6.5 Application information guide

Table 6-1 Application data

| Liquid | Chemical formula |
|--|--|
| | Name of liquid |
| | Concentration |
| | Density |
| | Viscosity at 20°C [cSt] |
| | Viscosity at process temperature [cSt] |
| Measurement range | |
| Nominal size [mm] | |
| Process temperature [°C] | |
| Ambient temperature (transmitter) [°C] | |
| Pressure [PN] | |
| Gas/solid content [%] | |
| Explosion protection | |

Table 6- 2 Sensor data

6.6 Return procedures

6.6 Return procedures

Enclose the delivery note, the cover note for return delivery together with the declaration of decontamination form on the outside of the package in a well-fastened clear document pouch.

Required forms

Delivery Note

• Cover Note for Return Delivery with the following information

Return delivery form (http://support.automation.siemens.com/WW/view/en/16604370)

- product (ordering number)
- number of devices or spare parts returned
- reason for the return
- Declaration of Decontamination

Decontamination declaration (<u>http://pia.khe.siemens.com/efiles/feldg/files/Service/declaration_of_decontamination_en.</u> pdf)

With this declaration you certify *that the returned products/spare parts have been carefully cleaned and are free from any residues.*

If the device has been operated together with toxic, caustic, flammable or waterdamaging products, clean the device before return by rinsing or neutralizing. Ensure that all cavities are free from dangerous substances. Then, double-check the device to ensure the cleaning is completed.

We shall not service a device or spare part unless the declaration of decontamination confirms proper decontamination of the device or spare part. Shipments without a declaration of decontamination shall be cleaned professionally at your expense before further proceeding.

You can find the forms on the Internet and on the CD delivered with the device.

| Description | 2-track sensor with four SONO 3200 transducers |
|------------------------------|---|
| Measurement accuracy at | v > 0.5 10 m/s, < ±0.5 % of flow rate |
| reference conditions | (v = flow velocity) |
| Max. flow velocity | 10 m/s (32 ft/s) |
| Nominal size | DN 100 1200 (4" 48") |
| Media/surface temperature | • Standard: −10 + 200 °C (14 392 °F) |
| | ATEX Ex-d version: : −20 + 180 °C (-4 356 °F) |
| | ATEX Ex-i version: : -10 + 190 °C (14 374 °F) |
| | Specials: -200 (-328 °F) or up to 250 °C (482 °F) |
| Ambient temperature (sensor) | • - 20 + 60 °C (-4 +140 °F) |
| | • Storage: - 40 +85 °C (-40 +185 °F) |
| Enclosure | Standard: IP68 (NEMA 6 / NEMA 6X) |
| | ATEX: According to certification |
| Transducer SONO 3200 | O-rings or flanges |

Table 7-1 Technical data SONO 3100

Table 7-2 Process connections

| Designation | Pipe material | |
|-------------------------------|-----------------|---|
| PN designated EN 1092-1 | Carbon steel | PN 10: DN 200DN 1200 (8" 48") PN 16: DN 100 DN 1200 (4" 48") PN 25: DN 200 1000 (8" 40") PN 40: DN 100 DN 500 (4" 20") |
| | Stainless steel | PN 10 and PN25: DN 200DN 300 (8" 12") PN 16 and PN 40: DN 100 DN 300 (4" 12") |
| Class designated EN 1759-1 | Carbon steel | Class 150: DN 100 DN 600 (4" 24") Class 300: DN 100 DN 300 (4" 12") |
| | Stainless steel | Class 150 and 300: DN 100 DN 300 (4" 12") |

| Designation | Pipe material | |
|-----------------------------------|---------------|--|
| Without flanges (weld-in version) | Carbon steel | PN 16: DN 100 DN 1200 (4" 48") |
| | | PN 25: DN 200 1000 (8" 40") |
| | | PN 40: DN 100 DN 500 (4" 20") |

Table 7-3 Materials

| Pipe | Carbon steel EN 1.0345, paintedStainless steel EN 1.4404 (AISI 316) |
|---------------------------|--|
| Flange (PN) | Carbon steel EN 1.0038Stainless steel EN 1.4404 (AISI 316) |
| Flange (Class) | ASTM A105ASTM F316L |
| Transducer body | Stainless steel: EN 1.4404 (AISI 316) or similar |
| Transducer terminal house | Stainless steel: EN 1.4404 (AISI 316)Polyamid: PA 6.6 |

Table 7-4 Certificates and approvals

| Declaration of conformity | CE declaration available on the internet and on the Sitrans F literature CD (supplied with the device). |
|---------------------------|---|
| Material certificate | Material certificate according to EN 10204-3.1 is available as option. |
| NDT examination report | Non Destructive Test (e.g. ultrasonic or penetrant test) available as option. |
| Pressure certificate | Pressure test according to EN 1024-2.3 is available as option. |
| Calibration report | A standard calibration report is supplied with the sensor.An extended accredited ISO/IEC 17025 calibration is available as option. |
| Ex approvals | Transmitter (FUS060): II 2G Ex dem [ia/ib] IIC T6/T4/T3 Sensor (SONO 3100 Ex-i approved version): II 2G Ex ib IIC T6/T4/T3 (only approved for use with FUS060 Ex-version) Sensor (SONO 3100 Ex d approved version): II 2G EEx d IIC T3-T6 (Only approved for use with FUS060 non Ex-version installed in safe zone) |

7.1 Coaxial cable specifications

Table 7-5 Technical data, Standard coaxial cable

| Standard Coaxial cable (75 Ω) | Coaxial cable with SMB straight plug on one end for the FUS060 connector |
|---------------------------------------|--|
| Outside diameter | Ø 5.8 mm |
| Length | 3, 15, 30, 60, 90, 120 m (9.84, 49.21, 98.43, 196.85, 295.28, 393.70 ft) between sensor and transmitter. |
| Material (outside jacket) | Black PE |
| Ambient temperature | -10 +70 °C (14 158 °F) |

Table 7-6 Technical data, HT coaxial cable

| High temperature Coaxial cable (75 Ω) | Coaxial cable with SMB straight plug on one end for the FUS060 connector |
|---|---|
| Outside diameter | Ø 5.13 mm (first 0.3 m (0.98 ft) of cable) Ø 5.8 mm (remaining cable) - with plug hot melt junction on the end) Between the two parts a mounted black hot melt junction Ø 16 mm (length 70 mm) |
| Length | 3, 15, 30, 60, 90, 120 m (9.84, 49.21, 98.43, 196.85, 295.28, 393.70 ft) between sensor and transmitter |
| Material (outside jacket) | Brown PTFE (first 0.3 m (0.98 ft) of cable)Black PE (remaining cable) |
| Ambient temperature | -200 +200 °C (-328 +392 °F) (first 0.3 m (0.98 ft)) -10 +70 °C (14 158 °F) (remaining cable) |

7.2 Pressure and temperature rating

The maximum permissible pressure and temperature for Siemens Flow Instruments ultrasonic flowmeters are indicated on the sensor label.

Flanges according to PN

Flanges and joints as well as related pressure/temperature (p/t) classification are described in EN 1092.

- For steel group 1E1: Table 15
- For material group 13E0: Table 17

7.3 Reference conditions

Flanges according to ANSI Class

Flanges and joints as well as related pressure/temperature (p/t) classification are described in EN 1759-1.

- For steel group 1.1 ASTM A105, class 150: Table 16
- For steel group 1.1 ASTM A105, class 300: Table 1

No flange bolts or gaskets are supplied. Bolts must comply with EN 1515-2 and gaskets with EN 1591-1.

WARNING

Exposing the sensors to pressures or temperatures above the limits stated may cause damage.

The sensor construction does not allow external action other than what is normal during common mounting in the pipeline. Make allowance for earthquakes, action of the air etc.

7.3 Reference conditions

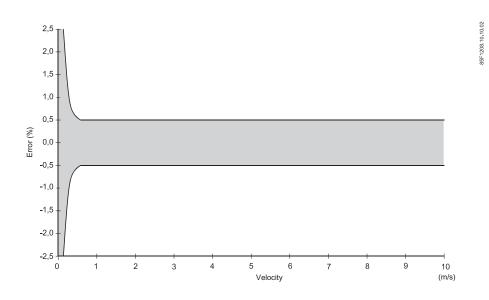


Figure 7-1 Reference condtions

| Fluid: | Water |
|----------------------|--|
| Fluid temperature: | 25 °C ± 5 °K (77 °F ± 9 °F) |
| Ambient temperature: | 25 °C ± 5 °K (77 °F ± 9 °F) |
| Supply voltage | 120230 V AC ± 15% (50/60 Hz) |
| (FUS060): | • 1930 V DC/ 2126 V AC |


7.4 Dimensions and Weight

| Installation conditions: | Upstream section > 20x DN and downstream section > 5x DN |
|--------------------------|--|
| Rangeability: | 0-1 m/s to 0-10 m/s |
| Repeatabilty: | Better than 0.25% in the range from 0.5 m/s to 10 m/s |

 Table 7-8
 Additional effects of deviations from reference conditions

| Current output: As pulse/frequency output plus ± 0.1% ± 20 μ A |
|--|
|--|

7.4 Dimensions and Weight

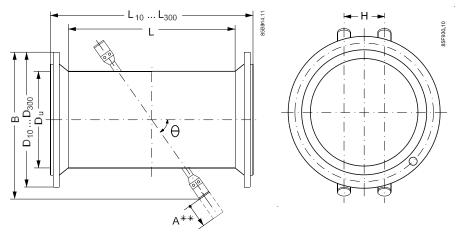

A**) Space required for replacement of transducer min. 230 mm (9,1 inch).

Table 7-9 SONO 3100 with EN norm

| PN | DN | Du | L1 | В | θ | Н | W ² | D | L1 | Weight** |
|----|------|--------|------|------|-----|-------|----------------|------|------|----------|
| | | (mm) | (mm) | (mm) | [°] | (mm) | (mm) | (mm) | (mm) | (kg) |
| 10 | 200 | 219.1 | 668 | 430 | 45* | 102.1 | 6.3 | 340 | 790 | 59 |
| | 250 | 273.0 | 714 | 480 | 45* | 127.6 | 6.3 | 395 | 850 | 73 |
| | 300 | 323.9 | 607 | 525 | 45* | 151.8 | 7.1 | 445 | 740 | 83 |
| | 350 | 355.6 | 639 | 550 | 45* | 166.4 | 8.0 | 405 | 770 | 98 |
| | 400 | 406.4 | 703 | 600 | 45* | 191.3 | 8.0 | 565 | 850 | 119 |
| | 500 | 508.0 | 797 | 690 | 45* | 241.1 | 7.1 | 670 | 950 | 153 |
| | 600 | 610.0 | 912 | 705 | 60 | 294.8 | 7.1 | 780 | 1075 | 193 |
| | 700 | 711.0 | 937 | 895 | 60 | 340.6 | 8.0 | 895 | 1100 | 262 |
| | 800 | 813.0 | 967 | 985 | 60 | 390.4 | 8.0 | 1015 | 1150 | 329 |
| | 900 | 914.0 | 1007 | 1070 | 60 | 445.9 | 10.0 | 1115 | 1200 | 428 |
| | 1000 | 1016.0 | 1060 | 1160 | 60 | 490.0 | 10.0 | 1230 | 1250 | 500 |
| | 1200 | 1220.0 | 1100 | 1350 | 60 | 588.0 | 8.0 | 1340 | 1280 | 680 |

7.4 Dimensions and Weight

| PN | DN | Du (mm) | L1 (mm) | B (mm) | θ [°] | H (mm) | W ² | D (mm) | L ¹ (mm) | Weight** (kg) |
|----|------|------------|------------|-----------|----------|-----------|----------------|-----------|------------------------|------------------|
| | | | | | | | (mm) | | | |
| 16 | 100 | 114.3 | 860 | 305 | 45* | 42.8 | 3.6 | 220 | 960 | 32 |
| | 125 | 139.7 | 862 | 325 | 45* | 64.5 | 4.0 | 250 | 970 | 38 |
| | 150 | 168.3 | 862 | 350 | 45* | 78.1 | 4.5 | 285 | 970 | 45 |
| | 200 | 219.1 | 668 | 430 | 45* | 102.1 | 6.3 | 340 | 790 | 58 |
| | 250 | 273.0 | 714 | 480 | 45* | 127.6 | 6.3 | 405 | 850 | 75 |
| | 300 | 323.9 | 607 | 525 | 45* | 151.8 | 7.1 | 460 | 760 | 92 |
| | 350 | 355.6 | 639 | 550 | 45* | 166.4 | 8.0 | 520 | 800 | 113 |
| | 400 | 406.4 | 703 | 600 | 45* | 191.3 | 8.0 | 580 | 875 | 141 |
| | 500 | 508.0 | 797 | 690 | 45* | 241.1 | 8.0 | 715 | 980 | 207 |
| | 600 | 610.0 | 912 | 705 | 60 | 294.8 | 8.8 | 840 | 1105 | 276 |
| | 700 | 711.0 | 937 | 895 | 60 | 340.6 | 8.8 | 910 | 1140 | 303 |
| | 800 | 813.0 | 967 | 985 | 60 | 390.4 | 10.0 | 1025 | 1180 | 400 |
| | 900 | 914.0 | 1007 | 1070 | 60 | 445.9 | 10.0 | 1125 | 1230 | 475 |
| | 1000 | 1016.0 | 1060 | 1160 | 60 | 490.0 | 10.0 | 1255 | 1300 | 594 |
| | 1200 | 1220.0 | 1100 | 1350 | 60 | 588.0 | 11.0 | 1455 | 1360 | 860 |
| 25 | 200 | 219.1 | 668 | 430 | 45* | 102.1 | 6.3 | 360 | 820 | 70 |
| | 250 | 273.0 | 714 | 480 | 45* | 127.6 | 7.1 | 425 | 890 | 96 |
| | 300 | 323.9 | 607 | 525 | 45* | 151.8 | 8.0 | 485 | 790 | 114 |
| | 350 | 355.6 | 639 | 550 | 45* | 166.4 | 8.0 | 555 | 840 | 145 |
| | 400 | 406.4 | 703 | 600 | 45* | 191.3 | 8.8 | 620 | 925 | 191 |
| | 500 | 508.0 | 797 | 690 | 45* | 241.1 | 10.0 | 730 | 1050 | 284 |
| | 600 | 610.0 | 912 | 705 | 60 | 294.8 | 11.0 | 845 | 1165 | 363 |
| | 700 | 711.0 | 937 | 895 | 60 | 340.6 | 12.5 | 960 | 1190 | 480 |
| | 800 | 813.0 | 967 | 985 | 60 | 390.4 | 14.2 | 1085 | 1240 | 650 |
| | 900 | 914.0 | 1007 | 1070 | 60 | 445.9 | 16.0 | 1185 | 1300 | 835 |
| | 1000 | 1016.0 | 1060 | 1160 | 60 | 490.0 | 17.5 | 1320 | 1370 | 1078 |
| 40 | 100 | 114.3 | 860 | 305 | 45* | 42.8 | 3.6 | 235 | 990 | 35 |
| | 125 | 139.7 | 862 | 325 | 45* | 64.5 | 4.0 | 270 | 990 | 44 |
| | 150 | 168.3 | 862 | 350 | 45* | 78.1 | 4.5 | 300 | 1010 | 52 |
| | 200 | 219.1 | 668 | 430 | 45* | 102.1 | 6.3 | 375 | 840 | 79 |
| | 250 | 273.0 | 714 | 480 | 45* | 127.6 | 7.1 | 450 | 920 | 117 |
| | 300 | 323.9 | 607 | 525 | 45* | 151.8 | 8.0 | 515 | 830 | 151 |
| | 350 | 355.6 | 639 | 550 | 45* | 166.4 | 8.8 | 580 | 880 | 191 |
| | 400 | 406.4 | 703 | 600 | 45* | 191.3 | 11.1 | 660 | 975 | 275 |
| | 500 | 508.0 | 797 | 690 | 45* | 241.1 | 14.2 | 755 | 1080 | 379 |

¹ Length tolerance (mm): DN100 +2/-3, DN125 to DN200 +3/-4, DN250 to DN400 +4/-5, DN500 to DN1200 +5/-6.

² Min. wall thickness for pressure rates PN10 to PN40.

* For all sensors with flange transducers the track angle is 60°.

**Weight of system incl. process flanges and standard o-ring transducers. For sensors with flange transducers please add appr. 10 kg (22,05 lbs). For SS terminal housings instead of the standard PA housing add appr. 5 kg (11,03 lbs).

7.4 Dimensions and Weight

| Class | DN (inch) | Du (inch) | L ¹ (inch) | B (mm) | θ [°] | Н | W ² (mm) | D (mm) | L ¹ (mm) | Weight** (Ibs) |
|-------|--------------|--------------|--------------------------|-----------|----------|--------|------------------------|-----------|------------------------|-------------------|
| | | | | | | (inch) | | | | |
| | | | | | | | | | | |
| 150 | 4 | 4.5 | 33.86 | 12.01 | 45* | 1.69 | 0.14 | 9.00 | 39.86 | 70.5 |
| | 5 | 5.5 | 33.94 | 12.80 | 45* | 2.54 | 0.15 | 10.00 | 40.94 | 83.8 |
| | 6 | 6.63 | 33.94 | 13.78 | 45* | 3.07 | 0.16 | 11.00 | 40.94 | 99.2 |
| | 8 | 8.63 | 26.30 | 16.93 | 45* | 4.02 | 0.16 | 13.50 | 34.30 | 127.9 |
| | 10 | 10.75 | 28.11 | 18.90 | 45* | 5.02 | 0.18 | 16.00 | 36.11 | 165.3 |
| | 12 | 12.75 | 23.90 | 20.67 | 45* | 5.98 | 0.20 | 19.00 | 32.90 | 202.8 |
| | 14 | 14.00 | 25.16 | 21.65 | 45* | 6.55 | 0.21 | 21.00 | 35.16 | 249.1 |
| | 16 | 16.00 | 27.68 | 23.62 | 45* | 7.53 | 0.22 | 23.50 | 33.74 | 310.9 |
| | 20 | 20.00 | 31.38 | 27.17 | 45* | 9.49 | 0.26 | 27.50 | 42.76 | 456.4 |
| | 24 | 24.00 | 35.91 | 27.76 | 60 | 11.61 | 0.30 | 32.00 | 47.91 | 608.5 |
| 300 | 4 | 4.5 | 33.86 | 12.01 | 45* | 1.69 | 0.25 | 10.00 | 40.62 | 77.2 |
| | 5 | 5.5 | 33.94 | 12.80 | 45* | 2.54 | 0.27 | 11.00 | 41.70 | 97.0 |
| | 6 | 6.63 | 33.94 | 13.78 | 45* | 3.07 | 0.30 | 12.50 | 41.70 | 114.6 |
| | 8 | 8.63 | 26.30 | 16.93 | 45* | 4.02 | 0.29 | 15.00 | 35.06 | 174.2 |
| | 10 | 10.75 | 28.11 | 18.90 | 45* | 5.02 | 0.34 | 17.50 | 37.35 | 257.9 |
| | 12 | 12.75 | 23.90 | 20.67 | 45* | 5.98 | 0.39 | 20.50 | 34.14 | 332.9 |

Table 7-10 SONO 3100 with ANSI norm

¹ Length tolerance (mm): 4"(DN100) +0,08"/-0,12"(+2/-3mm), 5"(DN125) to 8"(DN200) +0,12"/-0,16"(+3/-4mm) , 10"(DN250) to 16"(DN400) +0,16"/-0,20"(+4/-5mm), 20"(DN500) to 24"(DN600) +0,20"/-0,24"(+5/-6mm)).

² Minimum wall thickness for pressure rates CL150 or CL300.

 * For all sensors with flange transducers track angle are 60°

**Weight of system incl. process flanges and standard o-ring transducers. For sensors with flange transducers please add appr. 10 kg (22,05 lbs). For SS terminal housings instead of the standard PA housing add appr. 5 kg (11,03 lbs).

7.4 Dimensions and Weight

A

Appendix A

A.1 Sizing table (DN 100 to DN 1200)

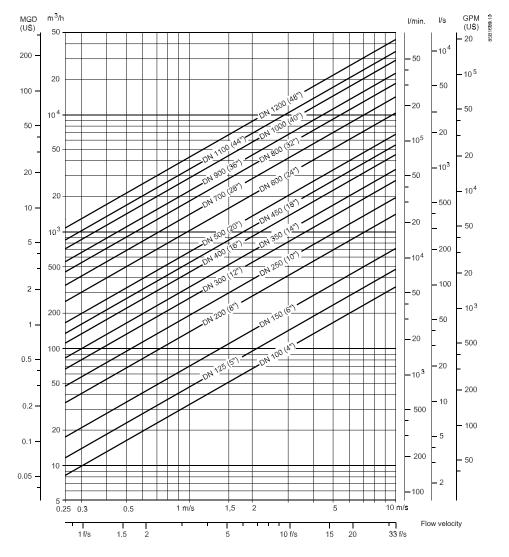


Figure A-1 Relationship between flow velocity V, flow quantity Q and sensor dimension DN.

Guidelines for sensor selection

- Min. measuring range: 0-1 m/s
- Max. measuring range: 0-10 m/s

Normally the sensor is selected so that V lies within the measuring range 1-3 m/s.

```
Appendix A
```

A.2 Ordering

Flow velocity calculation formula

 $V = \frac{1273.24 \text{ x } \text{Q } [\text{l/s}]}{\text{Di}^2[\text{mm}]} \quad [\text{m/s}] \text{ or } V = \frac{353.68 \text{ x } \text{Q } [\text{m}^3/\text{h}]}{\text{Di}^2[\text{mm}]} \quad [\text{m/s}]$

A.2 Ordering

In order to ensure that the ordering data you are using is not outdated, the latest ordering data is always available on the Internet: Process instrumentation catalog (http://www.siemens.com/processinstrumentation/catalogs)

Index

С

Certificates and approvals, 32 Compliance, 9 Connection Electrical, (See Electrical connection) Contact person, 8 Customer Support Hotline, 28

D

Decontamination, 29 Description, 13 Design, 13 Document history, 7

Ε

Electrical connection Basic requirements, 23 Transducer wiring, 23 Transmitter wiring, 25

F

Flow direction, 20 Flow factor, 16 Flow velocity, 16

Η

Hazardous area Approvals, 10 Safety requirements, 11 Temperature specifications, 10 Hotline, 28

I

Inlet / outlet conditions, 19 Installation Ambient conditions, 17 Free outlet, 18 Horizontal pipes, 21 Indoor/outdoor, 17 Large pipes, 20 Location, 18 Mounting of sensor, 21 Orientation, 21 Safety instructions, 17 U-shaped pipes, 18 Vertical pipes, 21 Internet Contact person, 8, 28 Flowdocumentation, 8 Support, 28 Introduction, 7 Items supplied, 7

L

Laws and directives, 9 Liquid Abrasive, 21 Containing particles, 21 Gas / air bubbles, 22

Μ

Maintenance, 27 Material compatibility, 9 Measuring principle, 15

Ρ

Pipe reducers, 20 Pressure Safety instructions, 17 Pressure classification, 33 Pressure specifications, 17 Process connections, 31

R

Recalibration, 27 Reference conditions, 34 Repair, 27 Return procedures, 29

SITRANS F US SONO 3100 Operating Instructions, 06/2010, A5E00814513-05

S

Safety Instrument safety standards, 9 Safety instructions Installation, 17 Safety notes, 9 Sensor location, 18 Sensor orientation, 21 Service, 27, 28 Application information, 28 SONO 3200, 14 Support, 28 System components, 13

Т

Technical data HT coaxial cable, 33 SONO 3100, 31 SONO 3200, 14 Standard coaxial cable, 32 Transducer, 14 Temperature classification, 33 Temperature specifications, 10, 17 Transit time, 16

W

Wiring, (See Electrical connection)

For more information...

www.siemens.com/flow

Siemens A/S Flow Instruments Nordborgvej 81 DK-6430 Nordborg Subject to change without prior notice Order No.: A5E00814513 Lit. No.: A5E00814513-05 © Siemens AG 06.2010 All rights reserved



www.siemens.com/processautomation