

Temperature/RH Smart Sensor (S-THB-M00x) Manual



The temperature/RH smart sensor is designed to work with smart sensor-compatible HOBO® data loggers and stations. All sensor parameters are stored inside the smart sensor, which automatically communicates configuration information to the logger without any programming, calibration or extensive user setup.

Temperature/RH Smart Sensor

Models: S-THB-M002
S-THB-M008

Accessories:

- Solar radiation shield (M-RSA or RS3-B)
- Replacement RH sensor (HUM-RHPCB-2)


Specifications

	Temperature	RH
Measurement Range	-40°C to 75°C (-40°F to 167°F)	0-100% RH at -40° to 75°C (-40° to 167°F); exposure to conditions below -20°C (-4°F) or above 95% RH may temporarily increase the maximum RH sensor error by an additional 1%
Accuracy	±0.21°C from 0° to 50°C (±0.38°F from 32° to 122°F); see Plot A	±2.5% from 10% to 90% RH typical to a maximum of ±3.5% including hysteresis at 25°C (77°F); below 10% and above 90% ±5% typical
Resolution	0.02°C at 25°C (0.04°F at 77°F); see Plot A	0.1% RH
Bits Per Sample	12	10
Drift	<0.1°C (0.18°F) per year	<1% per year typical
Response Time (typical, to 90% of change)	5 minutes in air moving 1 m/sec	5 minutes in air moving 1 m/sec with protective cap
Operating Temperature Range	-40°C to 75°C (-40°F to 167°F)	
Environmental Rating	Weatherproof: 0 to 100% RH intermittent condensing environments. For best results, the temp/RH smart sensor should be mounted inside a protective enclosure, such as a solar radiation shield.	
Housing	PVC cable jacket with ASA styrene polymer RH sensor cap; modified hydrophobic polyethersulfone membrane	
Sensor Dimensions	10 x 35 mm (0.39 x 1.39 in)	
Weight	S-THB-M002: 110 g (3.88 oz); S-THB-M008: 180 g (6.35 oz)	
Number of Data Channels*	2	
Measurement Averaging Option	No	
Cable Lengths Available	2.5 m (8.2 ft); 8 m (26.2 ft)	
Length of Smart Sensor Network Cable*	0.5 m (1.6 ft); 6 m (19.6 ft)	



The CE Marking identifies this product as complying with all relevant directives in the European Union (EU).

* A single HOBO station can accommodate 15 data channels and up to 100 m (328 ft) of smart sensor cable (the digital communications portion of the sensor cables).

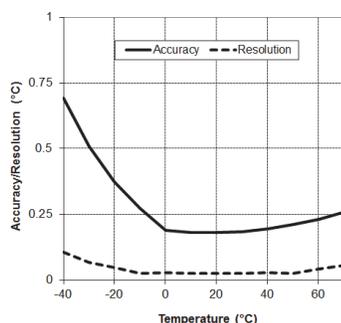


Plot A: Temperature Accuracy and Resolution


Mounting

Typical Mounting

Solar Radiation Shield: Use the washer and screw (included with the M-RSA radiation shield) or cable clamps (included with the RS3-B radiation shield) to secure the smart sensor in the radiation shield as shown at right and below.

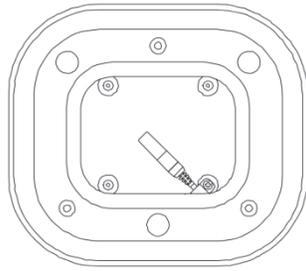


Temp/RH Sensor mounted in the Solar Radiation Shield M-RSA

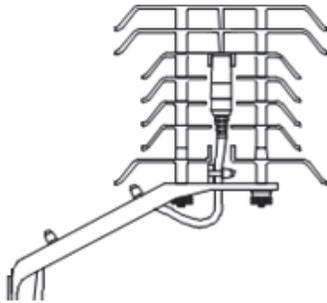

Temp/RH Sensor mounted in Solar Radiation Shield RS3-B (cross-section)

Mounting Considerations

- A solar radiation shield is strongly recommended when measuring air temperature in direct sunlight. Solar radiation can be a significant source of error in the temperature and RH readings.
- When mounting the probe, care should be taken to thermally isolate the sensor from the mounting surface to ensure accurate air temperature and humidity readings. The probe's temperature sensor is at the end of the cable, just below the cap.
- It is recommended that the probe be protected from direct exposure to the weather. This will prolong the sensor accuracy.
- Secure the smart sensor adapter to the mast with the cable ties as shown. Multiple smart sensor adapters can be stacked as shown in the example below on the right.

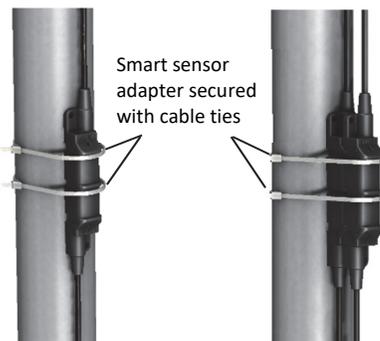

One Smart Sensor Adapter Mounted

Two Smart Sensor Adapters Stacked and Mounted

Alternatively, mount the smart sensor adapter to a flat surface using two screws (no larger than a #6) and two washers as shown at right.



- If you are running sensor cables along the ground, it is recommended that you use conduit to protect against animals, lawn mowers, exposure to chemicals, and so on.
- Refer to the station manual and Tripod Setup Guide for more information regarding setting up stations.


Connecting the Sensor to a Station or Logger

To connect the sensor to a station or logger, stop the station or logger from logging and insert the smart sensor's modular jack into an available smart sensor port. See the station manual for details on operating stations or loggers with smart sensors.

Replacing the RH Sensor

The RH sensor is protected by an ASA styrene polymer cap and a modified hydrophobic polyethersulfone fluid barrier membrane that allows vapor to penetrate while protecting the sensor from condensation. RH sensor performance may degrade over time. To replace the RH sensor, take the following steps:

1. Remove the tape fastening the sensor cap to the receptacle. Discard the tape.
2. Grasp the cap and membrane and pull firmly to remove them. Discard them.
3. **Note the orientation of the small circuit board containing the RH sensor.** Pull it out and discard it in compliance with local disposal guidelines for circuit boards.

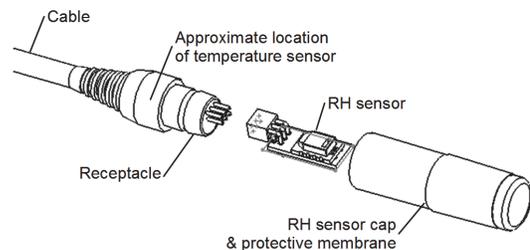

4. Push gently but firmly to install the new sensor (HUM-RHPCB-2) **in the same orientation.**
5. Put the new sensor cap and membrane on. Do not force the cap. If it does not go on easily, the sensor may be installed backwards. Reverse the sensor and try again.

Maintenance

The temperature/RH smart sensor is sensitive to dust, salts and other airborne contamination. Periodically inspect the RH sensor. If contamination is present on the protective cap, gently rinse it with cool fresh water. If the sensor itself is contaminated, you can rinse it with distilled water. Do not use hot water, organic solvents, or detergents. Dry before use.